

Sample Received: **April 15, 2026**

COA Issued: **April 18, 2026**

## PRODUCT INFORMATION

Vendor: <b>Vivo Peptides</b>	Sample Name: <b>KLOW 80mg</b>	Sample Type: <b>Blue lyophilized powder</b>	Lot Number: <b>VP-2025-0612</b>	MW: <b>342, 403, 1419, 4964 g/mol</b>
---------------------------------	----------------------------------	--	------------------------------------	--

## ANALYTICAL METHODS

**Identity:** Confirmed via MALDI-MS




**Purity:** RP-HPLC (214 nm)

**Content:** HPLC quantitation

## TEST RESULTS

Specification	Result	Method	Status
Identity: KLOW	GHK-Cu, KPV, BPC-157 & TB -500	MALDI-MS	✓ Conforms
Content	50.23, 10.18, 11.37, 9.84 mg	HPLC Quantitation	✓ Conforms
Overall Purity	99.8 %	RP-HPLC (214 nm)	✓ Conforms

HPLC Chromatogram (Retention Time: 2.13, 2.46, 4.52, 6.07 min)

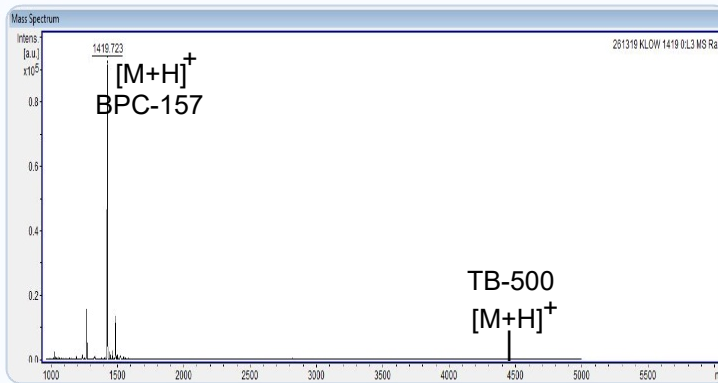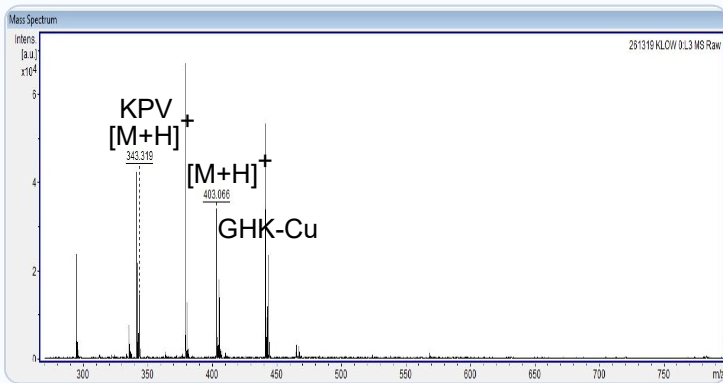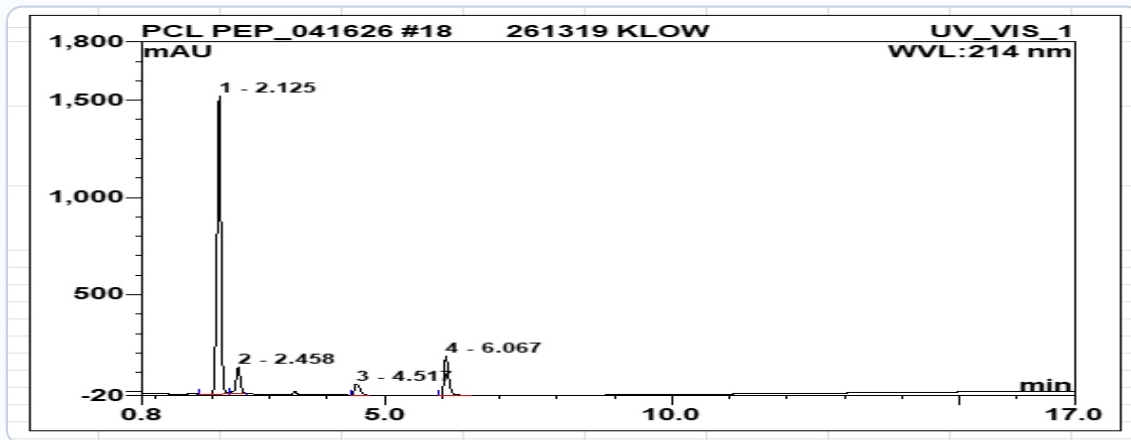

**Certification:** This COA confirms that the tested material meets or exceeds Bioviridian's analytical quality specifications for peptide research use.

Visit: <https://bioviridians.com/coa-search.html>



*Shane Straight*

**Shane Straight, M.S.**  
Principal Chemist, Bioviridian Inc.